

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Patent Number: 7,357,792
Issued: April 15, 2008
Name of Patentee: Newton et al.

Title of Invention: Positive Push Medical Valve With Internal Seal

Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

**REQUEST FOR CERTIFICATE OF CORRECTION OF PATENT
FOR PTO MISTAKE (37 C.F.R. § 1.322(a))**

1. Attached is PTO/SB/44 (also Form PTO-1050) in a form suitable for printing.
2. The exact page and line number where the errors are shown correctly in the application file are:

Please see "Petition for Submission of Formal Drawings Prior to Publication of Application" dated January 6, 2004, and USPTO's letter dated February 27, 2004 stating the replacement drawings will be included for patent publication. Copies of both are attached.

3. Please send the Certificate to:

Name: George J. Jakobsche
Address: Bromberg & Sunstein LLP
125 Summer Street
Boston, MA 02110-1618

/George J. Jakobsche, Reg. #39,236
George J. Jakobsche, Attorney of Record
Reg. No. 39,236
Phone: (617) 443-9292
Fax: (617) 443-0004

01600/00162 895400.1

UNITED STATES PATENT AND TRADEMARK OFFICE CERTIFICATE OF CORRECTION

Page 1 of 1

PATENT NO. : 7,357,792

APPLICATION NO.: 10/687,515

ISSUE DATE : April 15, 2008

INVENTOR(S) : Brian L. Newton, et al.

It is certified that an error appears or errors appear in the above-identified patent and that said Letters Patent is hereby corrected as shown below:

Figures 1-7 (Formal Drawings are attached)

MAILING ADDRESS OF SENDER (Please do not use customer number below):

George J. Jakobsche
Bromberg & Sunstein LLP
125 Summer Street
Boston, MA 02110-1618

1

This collection of information is required by 37 CFR 1.322, 1.323, and 1.324. The information is required to obtain or retain a benefit by the public which is to file (and by the USPTO to process) an application. Confidentiality is governed by 35 U.S.C. 122 and 37 CFR 1.14. This collection is estimated to take 1.0 hour to complete, including gathering, preparing, and submitting the completed application form to the USPTO. Time will vary depending upon the individual case. Any comments on the amount of time you require to complete this form and/or suggestions for reducing this burden, should be sent to the Chief Information Officer, U.S. Patent and Trademark Office, U.S. Department of Commerce, P.O. Box 1450, Alexandria, VA 22313-1450. DO NOT SEND FEES OR COMPLETED FORMS TO THIS ADDRESS. **SEND TO: Attention Certificate of Corrections Branch, Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450.**

If you need assistance in completing the form, call 1-800-PTO-9199 and select option 2.

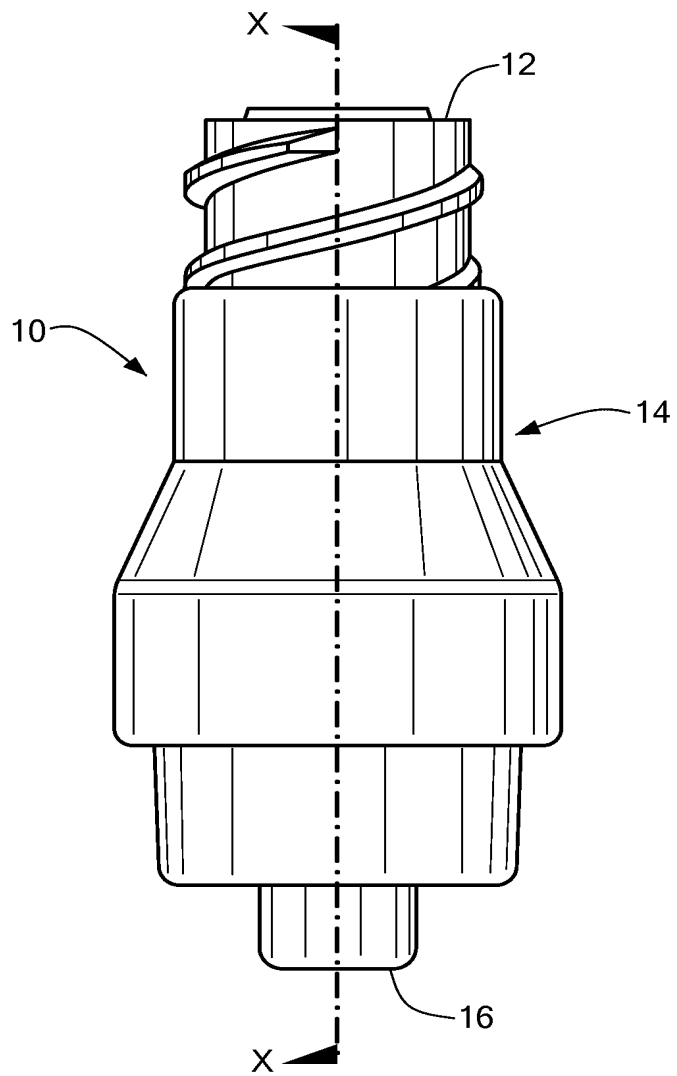
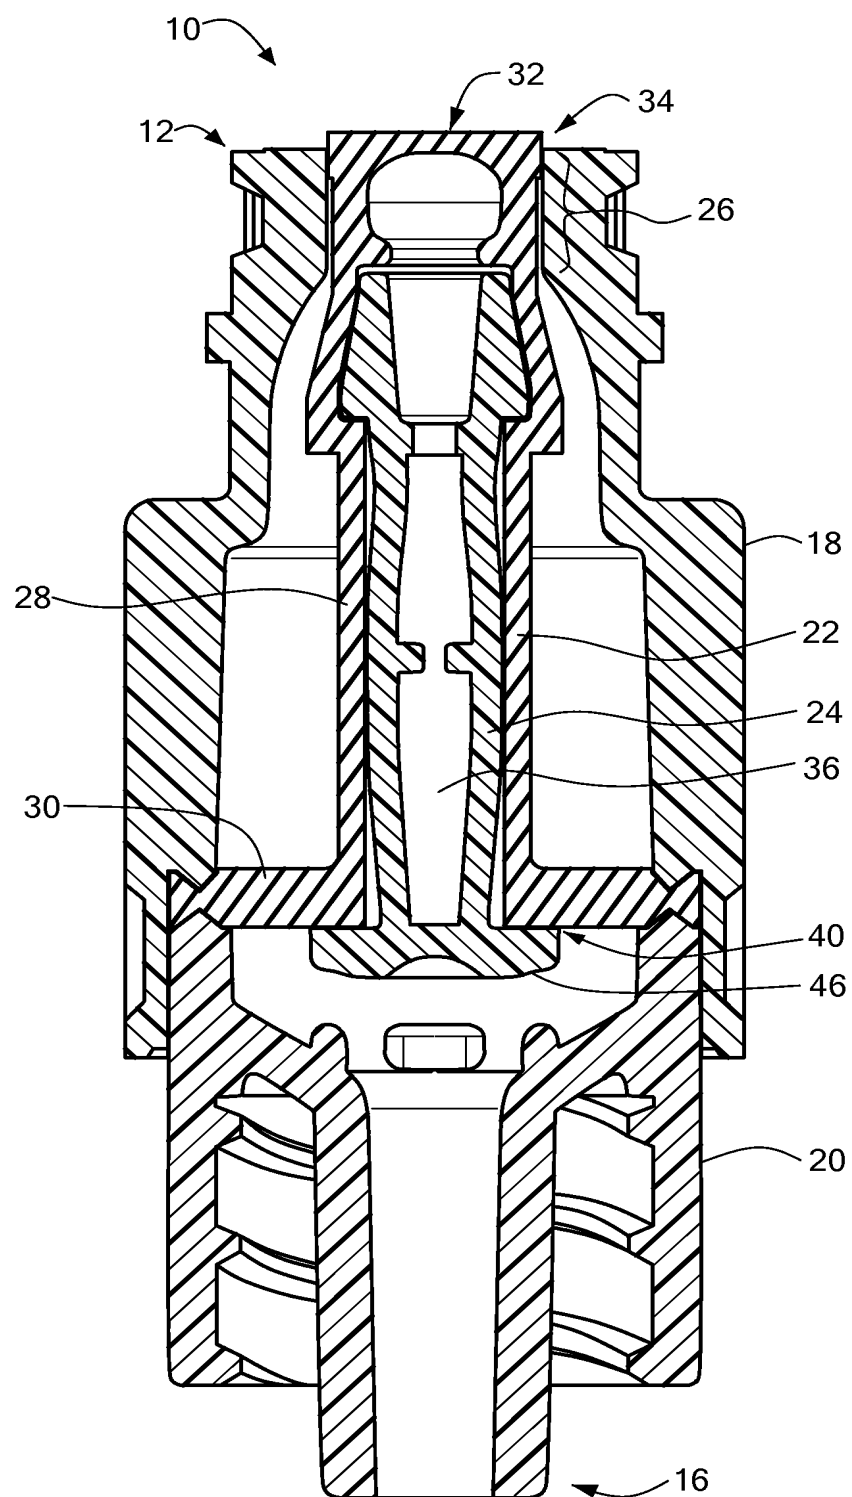


FIG. 1

**FIG. 2A**

3/9

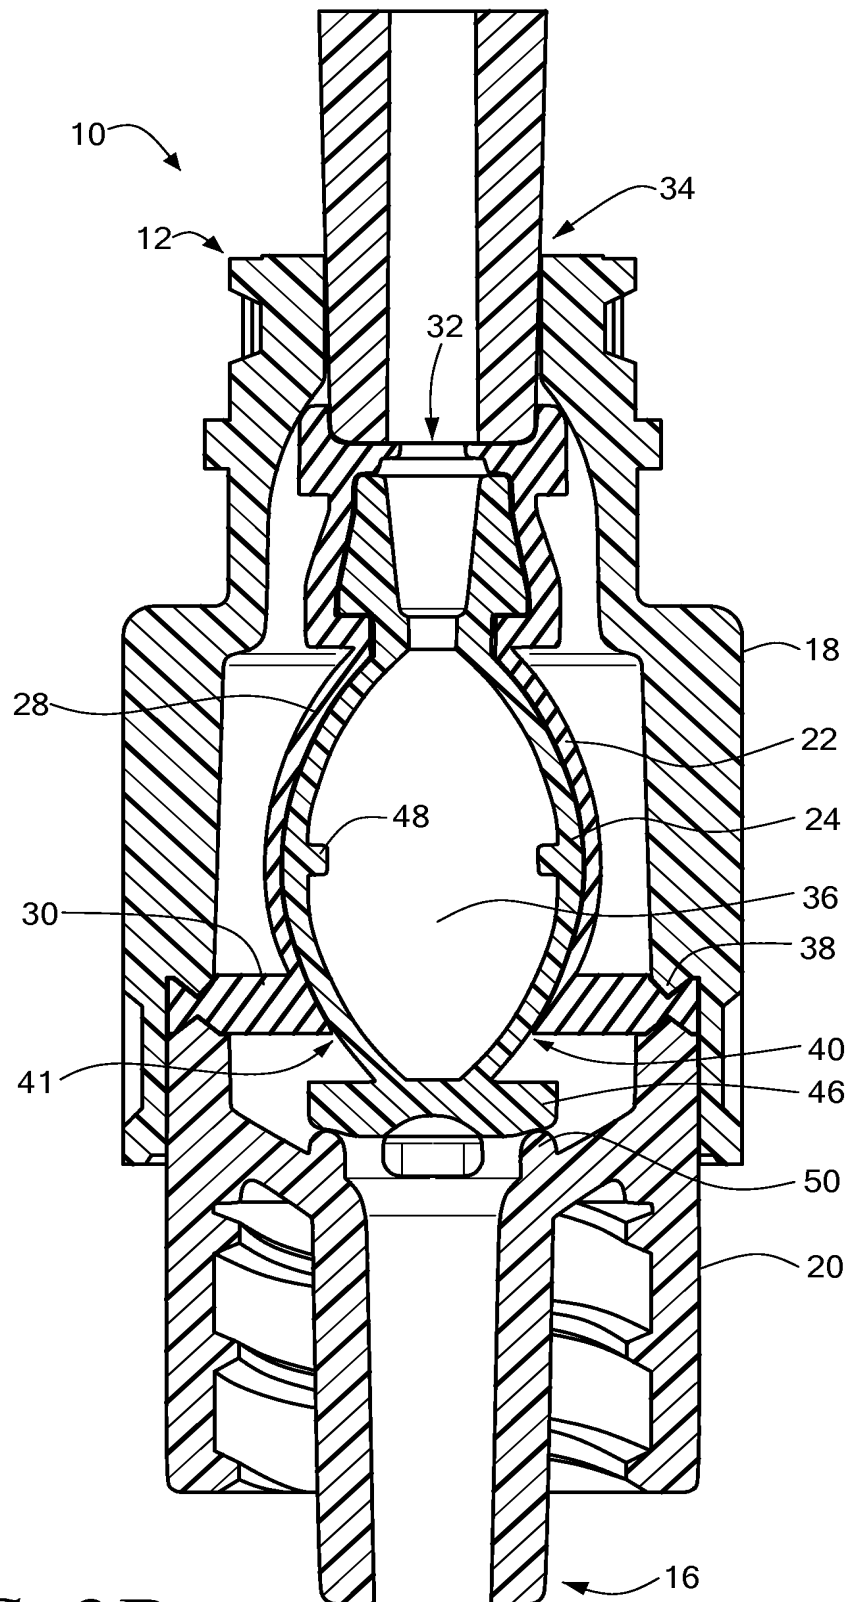


FIG. 2B

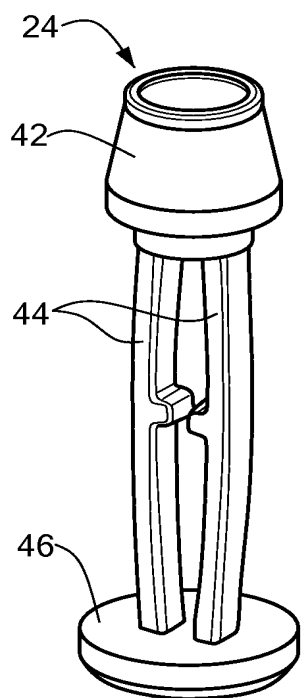


FIG. 3

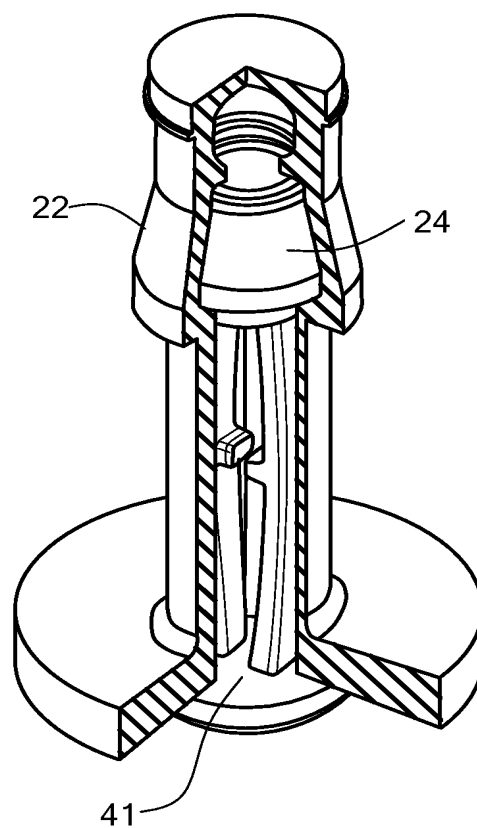


FIG. 4

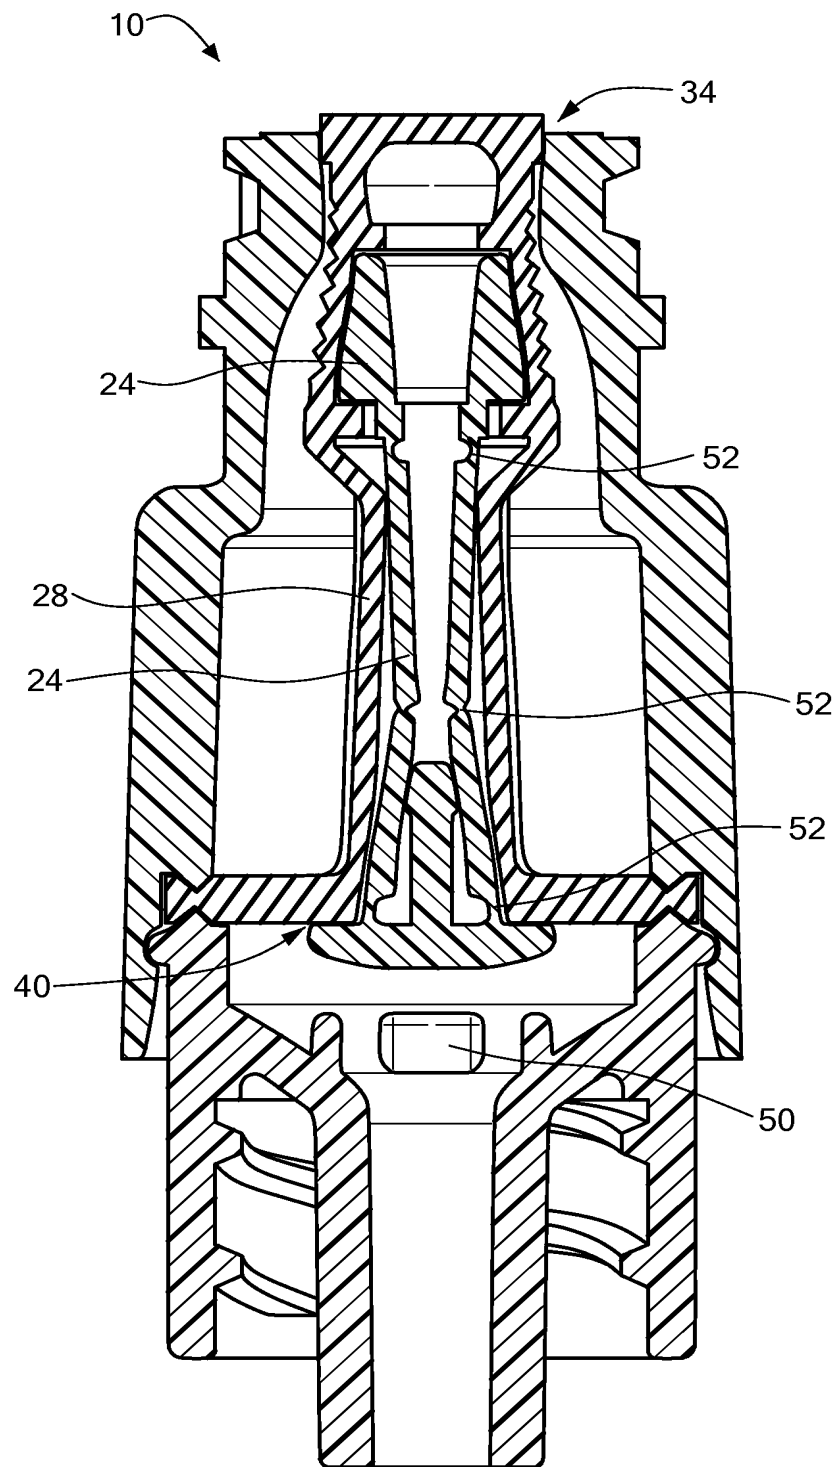
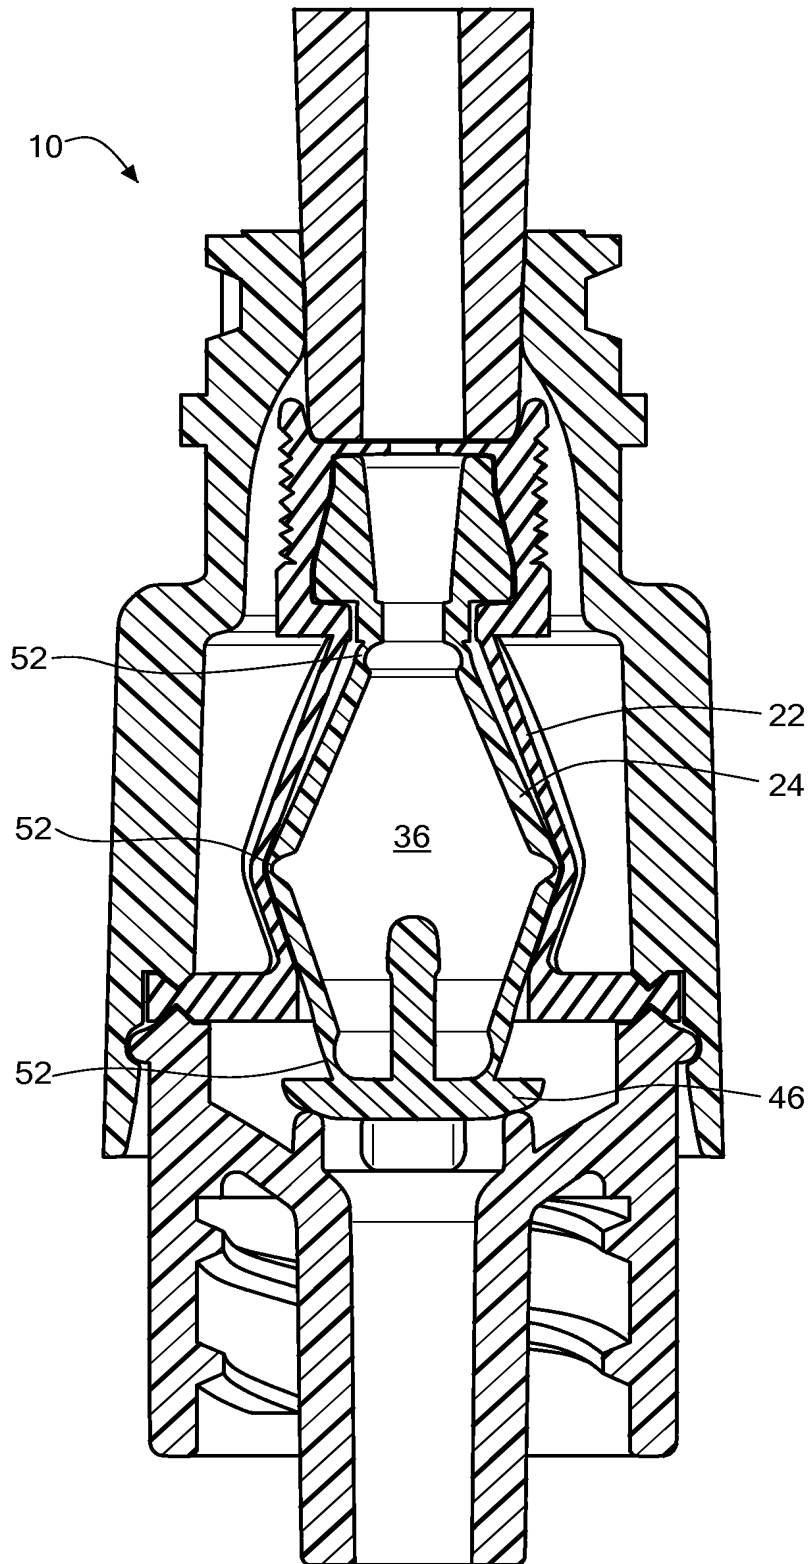
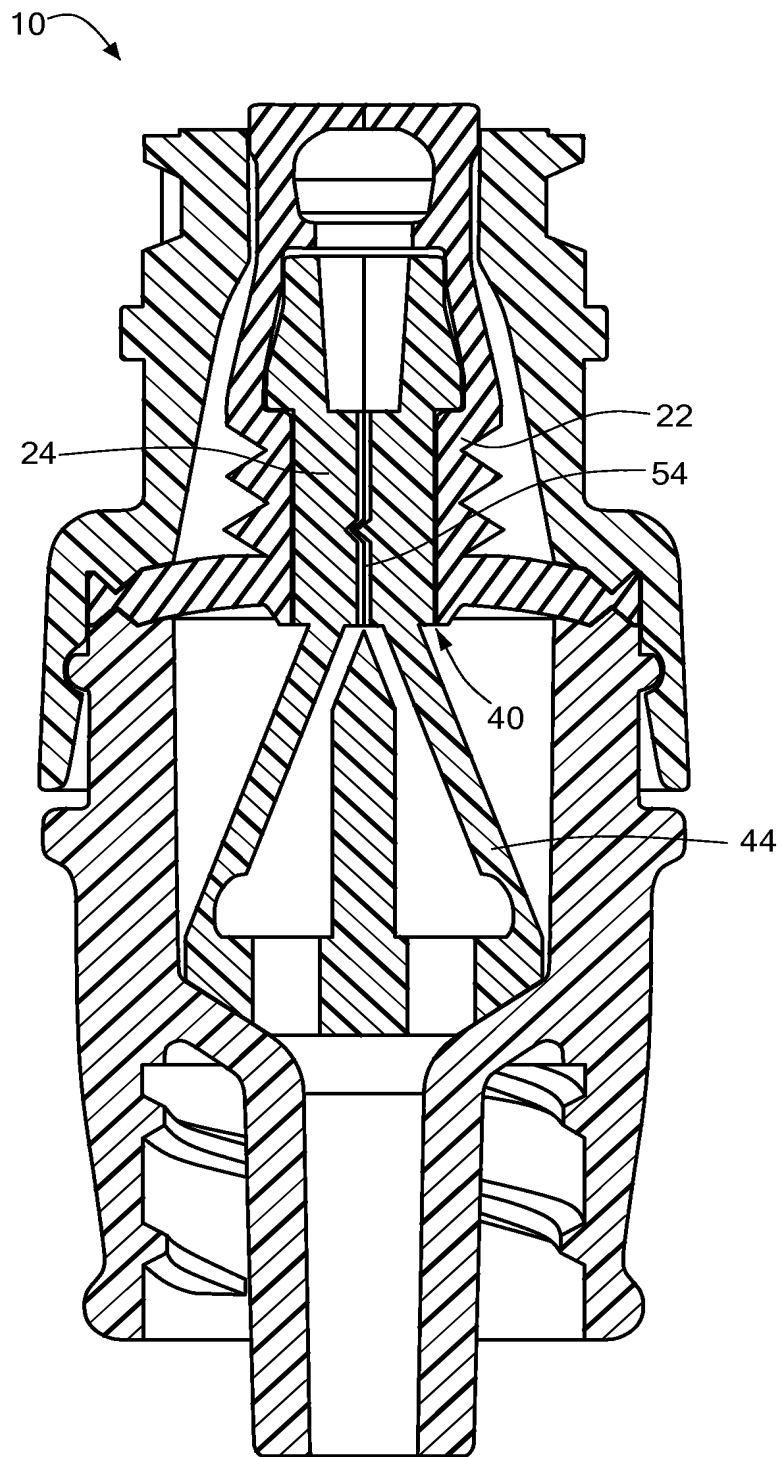


FIG. 5A

***FIG. 5B***

***FIG. 6A***

8/9


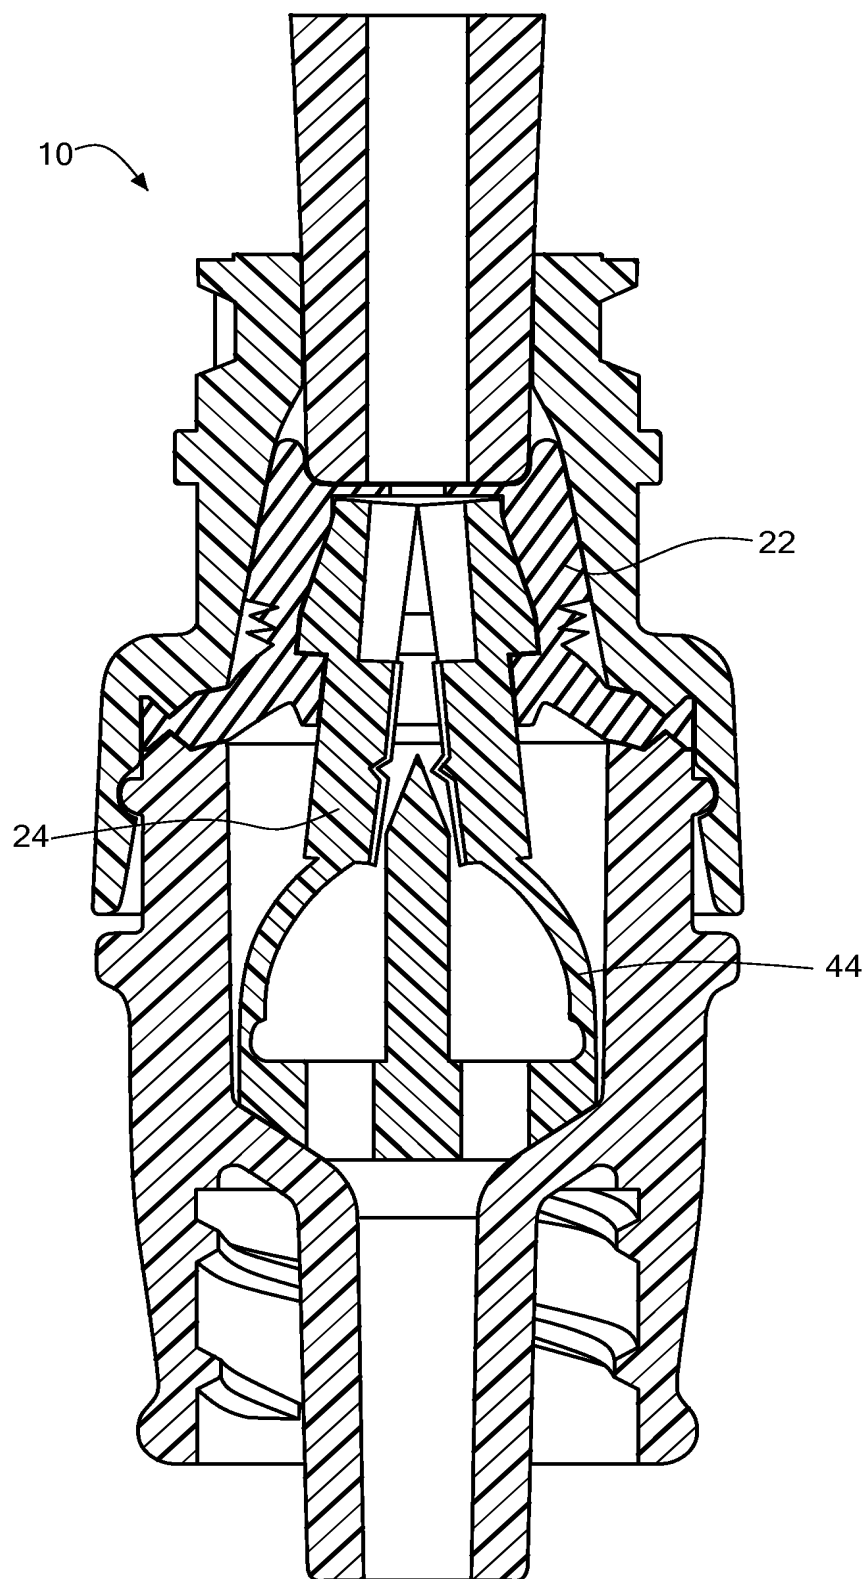


FIG. 6B

**FIG. 7**

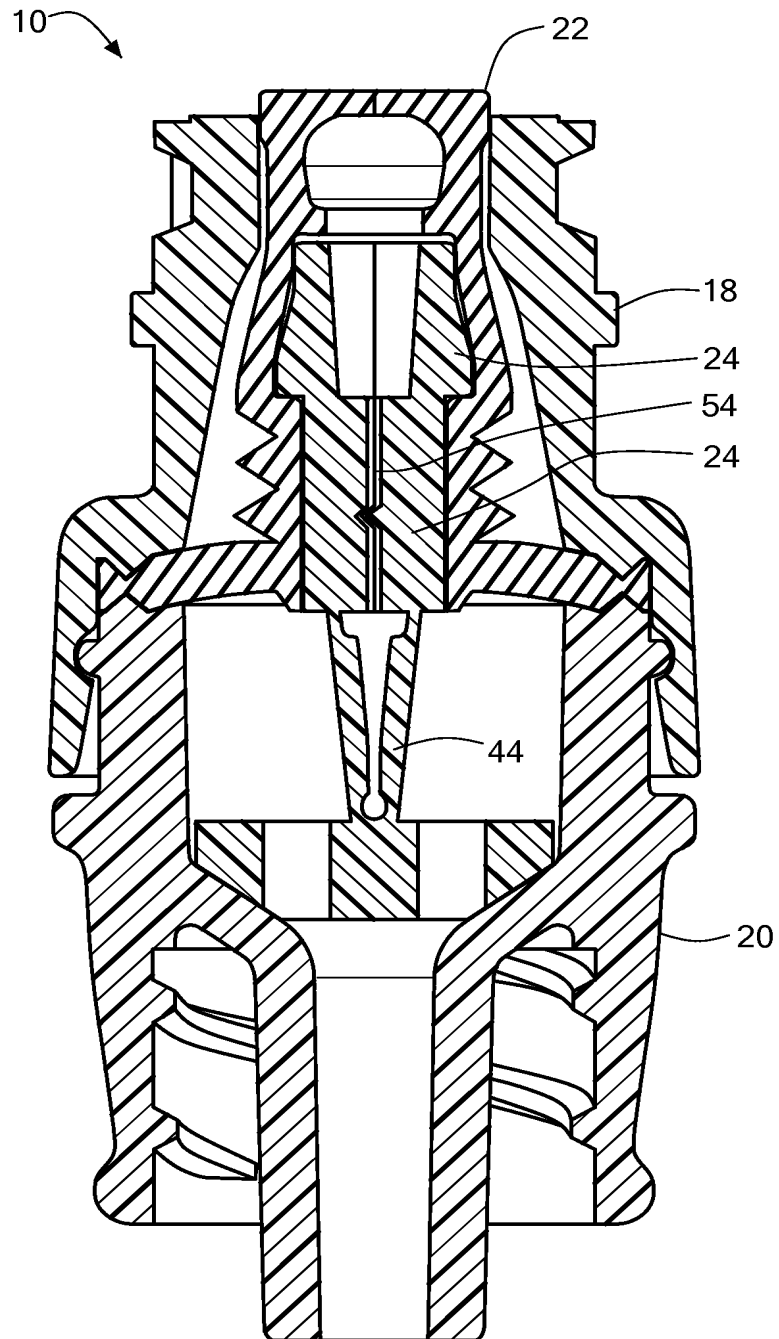

United States
Patent And
Trademark Office

DOCKETED

P.O. Box 1450, Alexandria, Virginia 22313-1450 -- www.uspto.gov

PETITION DECISION

02/27/04

Steven G Saunders
Bromberg & Sunstein LLP
125 Summer Street
Boston, MA 02110-1618

Dear Applicant:

The Box PGPub replacement drawings for application number 10/687515 received on 01/06/04 by the U. S. Patent and Trademark Office will be included for patent publication.

Telephone inquiries should be directed to Kaletus King, Office of Pre-Grant Publication 703 605-4283.

Signature of Reviewer, Office of Pre-Grant Publication

IN THE UNITED STATES PATENT AND TRADEMARK OFFICE

Applicant:	Newton et al.	Atty. Docket:	1600/162
Serial No.:	10/687,515	Art Unit:	Not Yet Assigned
Date Filed:	October 16, 2003	Examiner:	Not Yet Assigned
Invention:	Positive Push Medical Valve	Filing Date:	January 6, 2004

DOCKETED

Certificate of Mailing Under 37 CFR §1.10

I hereby certify that this correspondence is being deposited with the United States Postal Service "Express Mail Post Office to Addressee" service under 37 CFR 1.10 in an envelope addressed to: MAIL STOP PGPUB DRAWINGS, Commissioner for Patents, P.O. Box 1450, Alexandria, VA 22313-1450 on the date indicated below.

Date: January 6, 2004


Steven G. Saunders

EV 333084134 US
Express Mail Label Number

MAIL STOP PGPUB DRAWINGS
Commissioner for Patents
P.O. Box 1450
Alexandria, VA 22313-1450

PETITION FOR SUBMISSION OF FORMAL DRAWINGS
PRIOR TO PUBLICATION OF APPLICATION


Dear Sir:

Pursuant to 37 CFR § 1.182, Applicants hereby petition to replace the informal drawings, presently on file, with the enclosed nine (9) sheets of formal drawings for Figures 1-7, prior to the publication of the application. Please charge the petition fee of \$130 set forth in 37 CFR § 1.17 (h) to Deposit Account No. 19-4972.

No additional fees are believed to be due in connection with this petition. However, please charge any additional fees to Deposit Account No. 19-4972.

Respectfully submitted,

BROMBERG & SUNSTEIN LLP

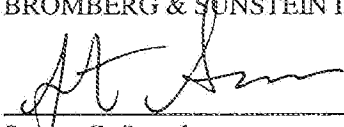
Steven G. Saunders
Registration No. 36,265
Attorney for Applicants

Date: January 6, 2004

BROMBERG & SUNSTEIN LLP
125 Summer Street
Boston, MA 02110-1618
(617) 443-9292
(617) 443-0004 (Facsimile)

01600/00162 288097.1

1/9

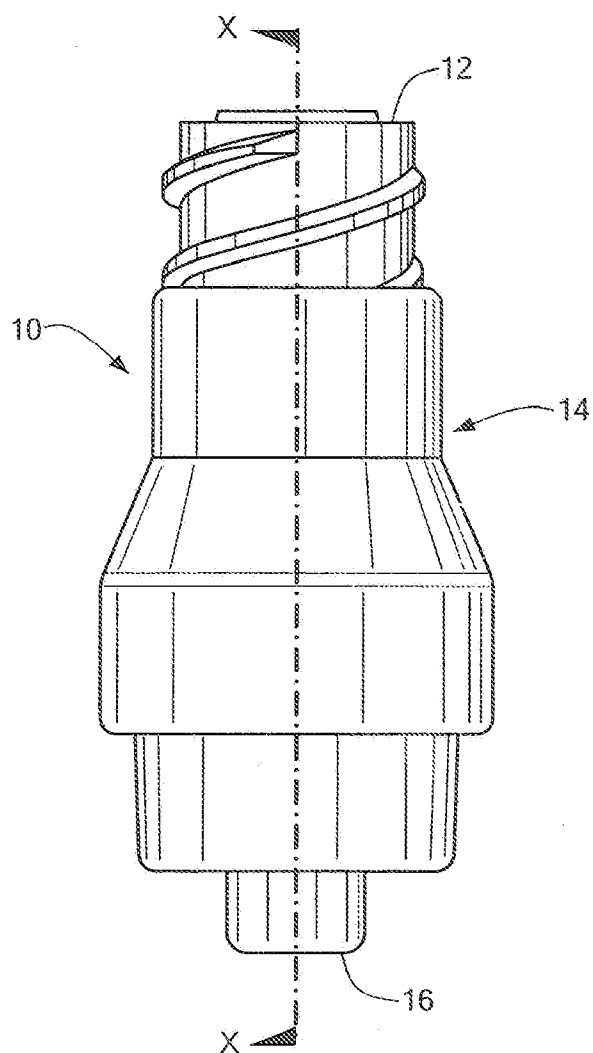


FIG. 1

2/9

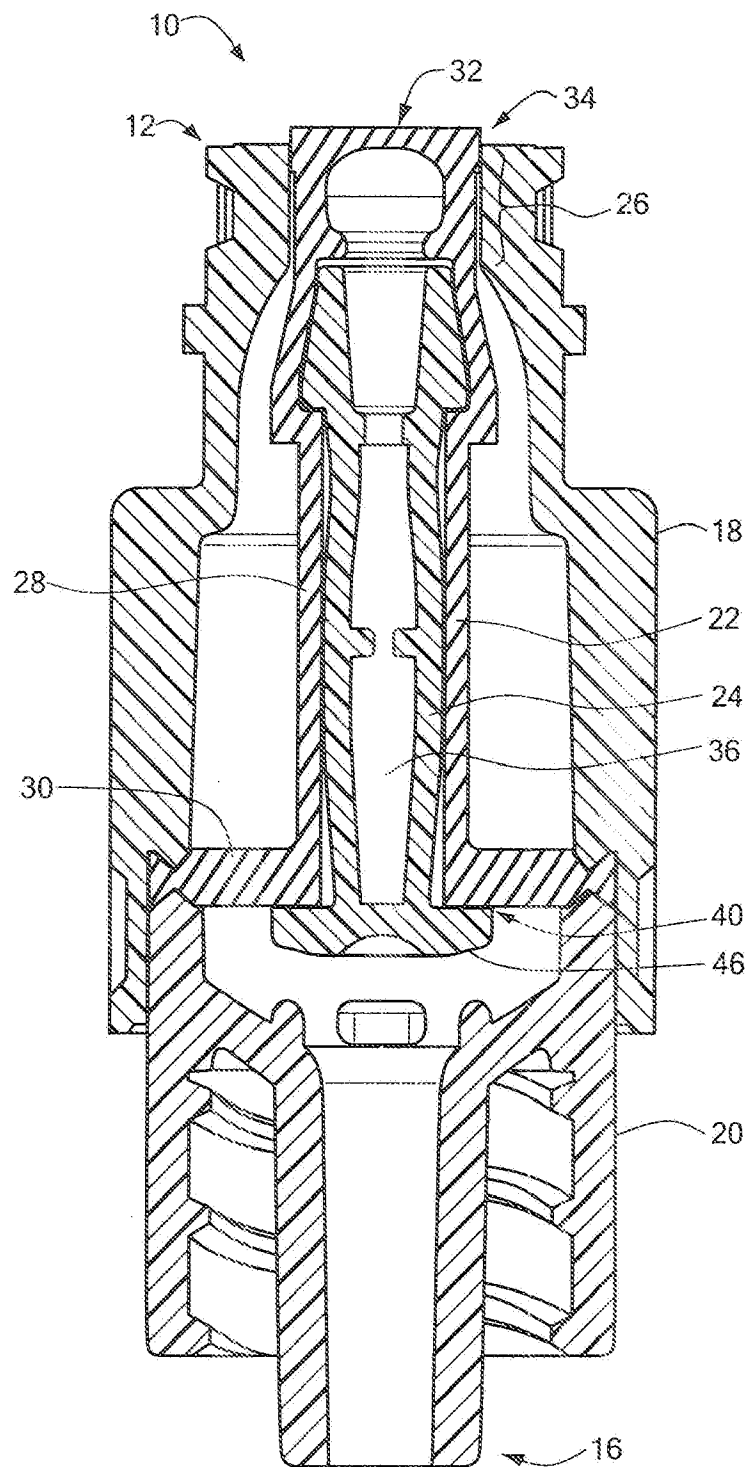


FIG. 2A

3/9

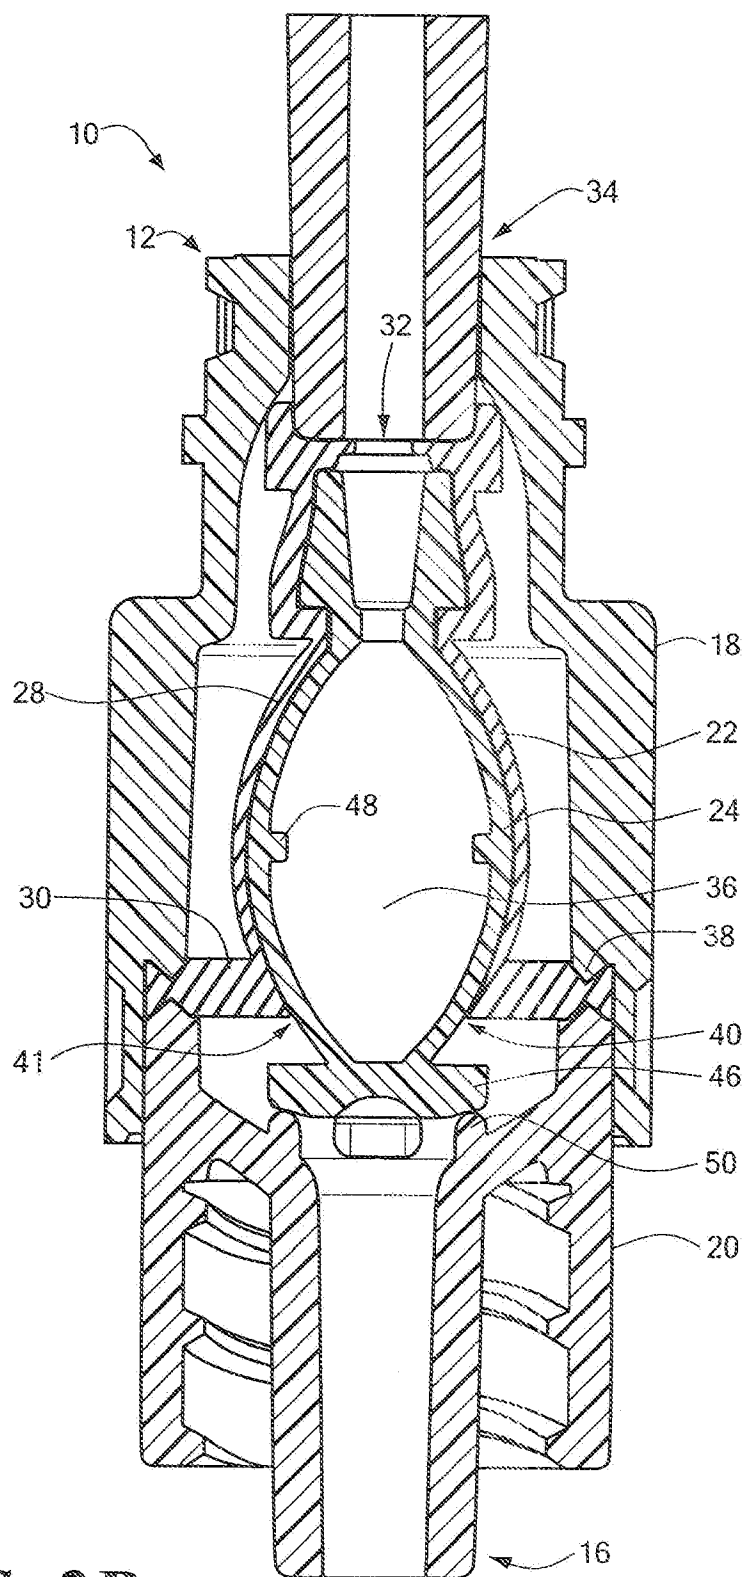


FIG. 2B

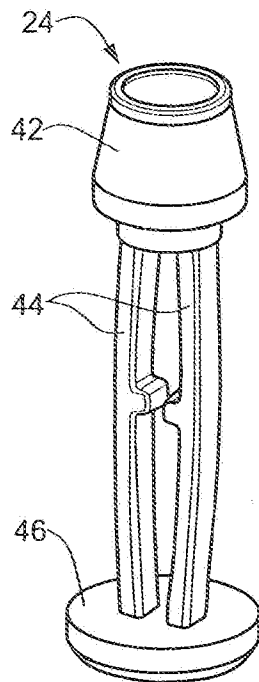


FIG. 3

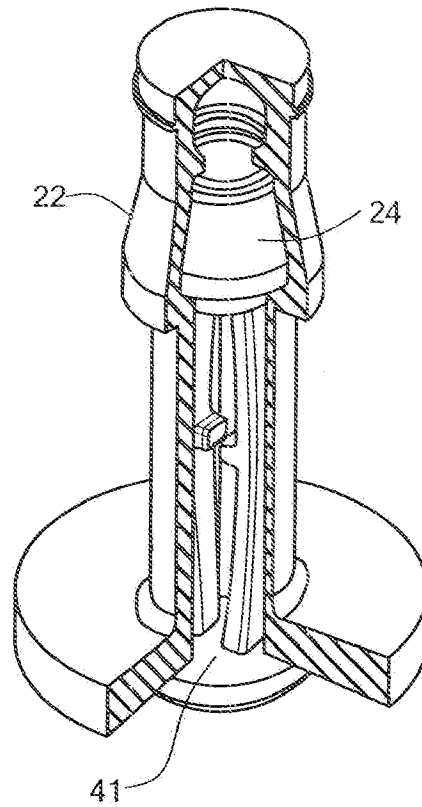


FIG. 4

5/9

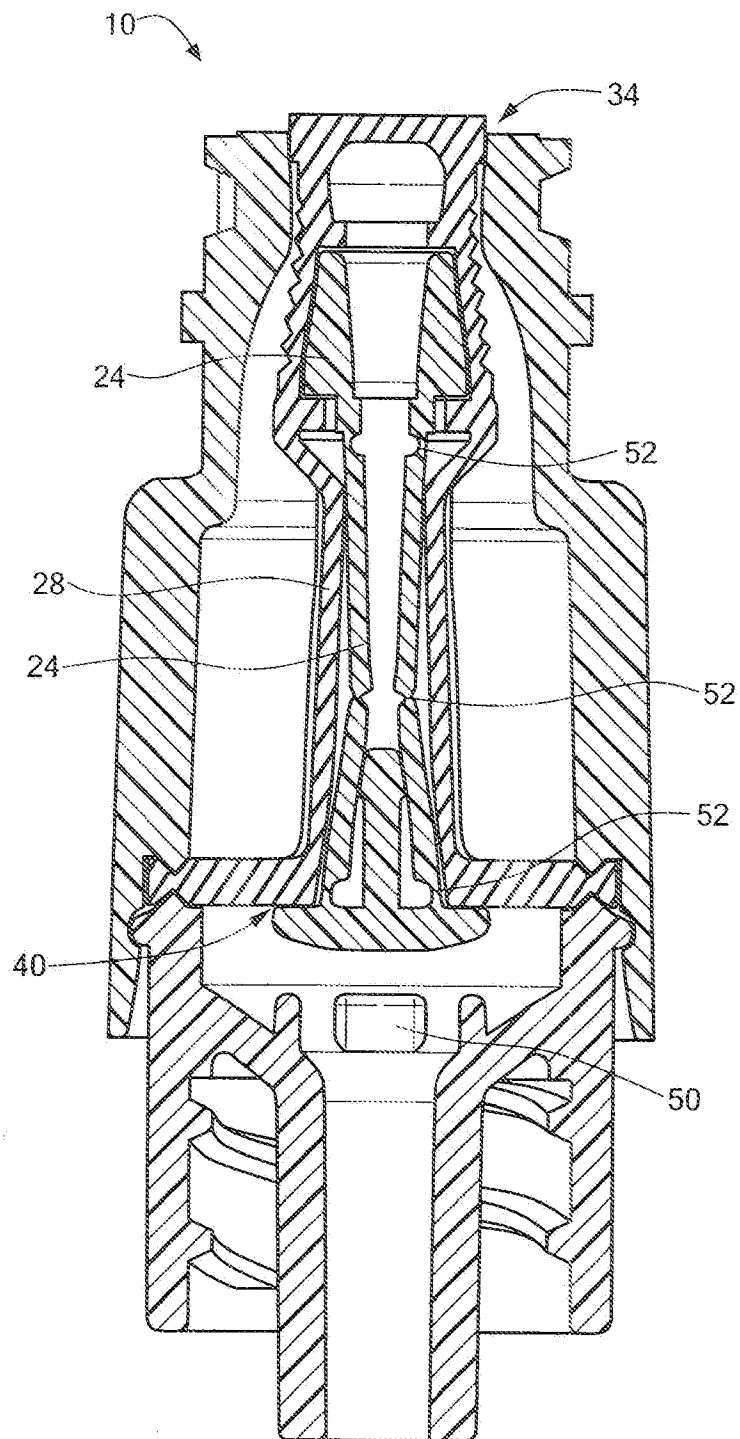


FIG. 5A

6/9

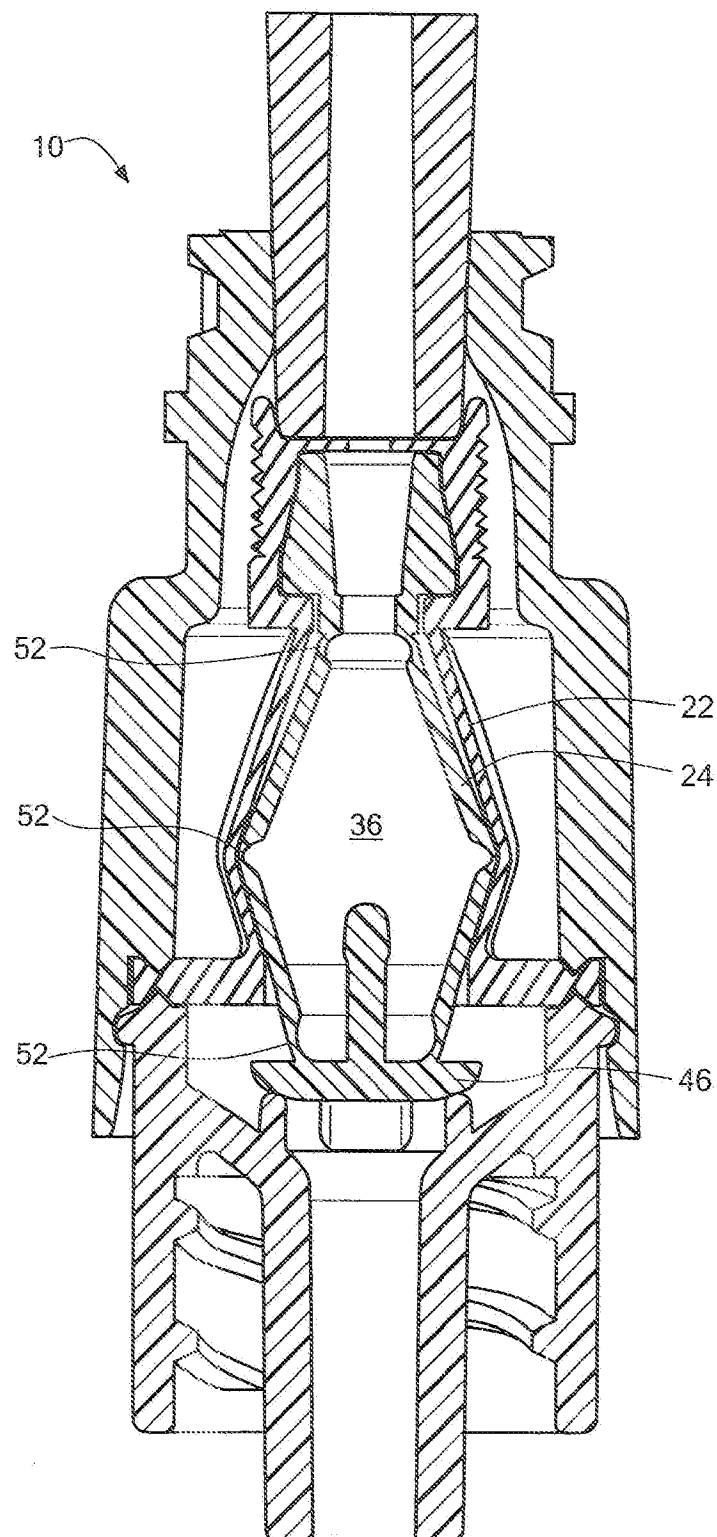


FIG. 5B

7/9

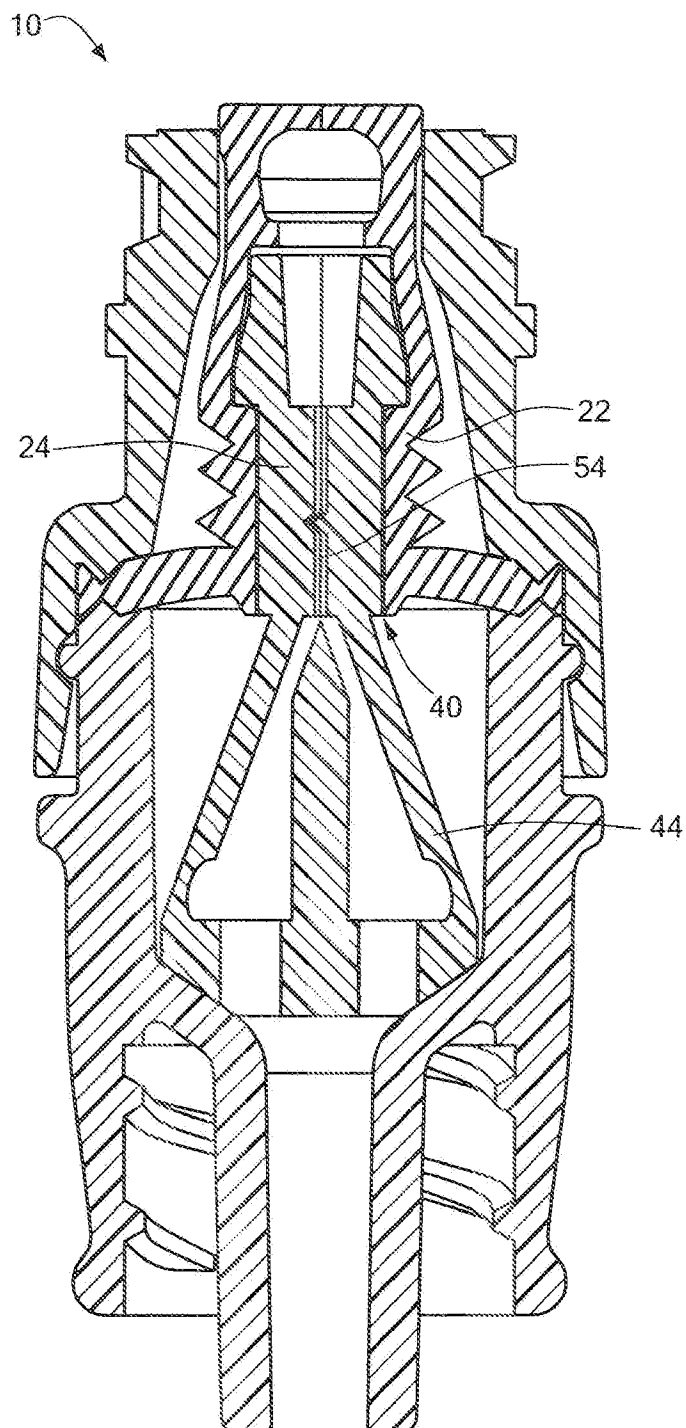


FIG. 6A

8/9

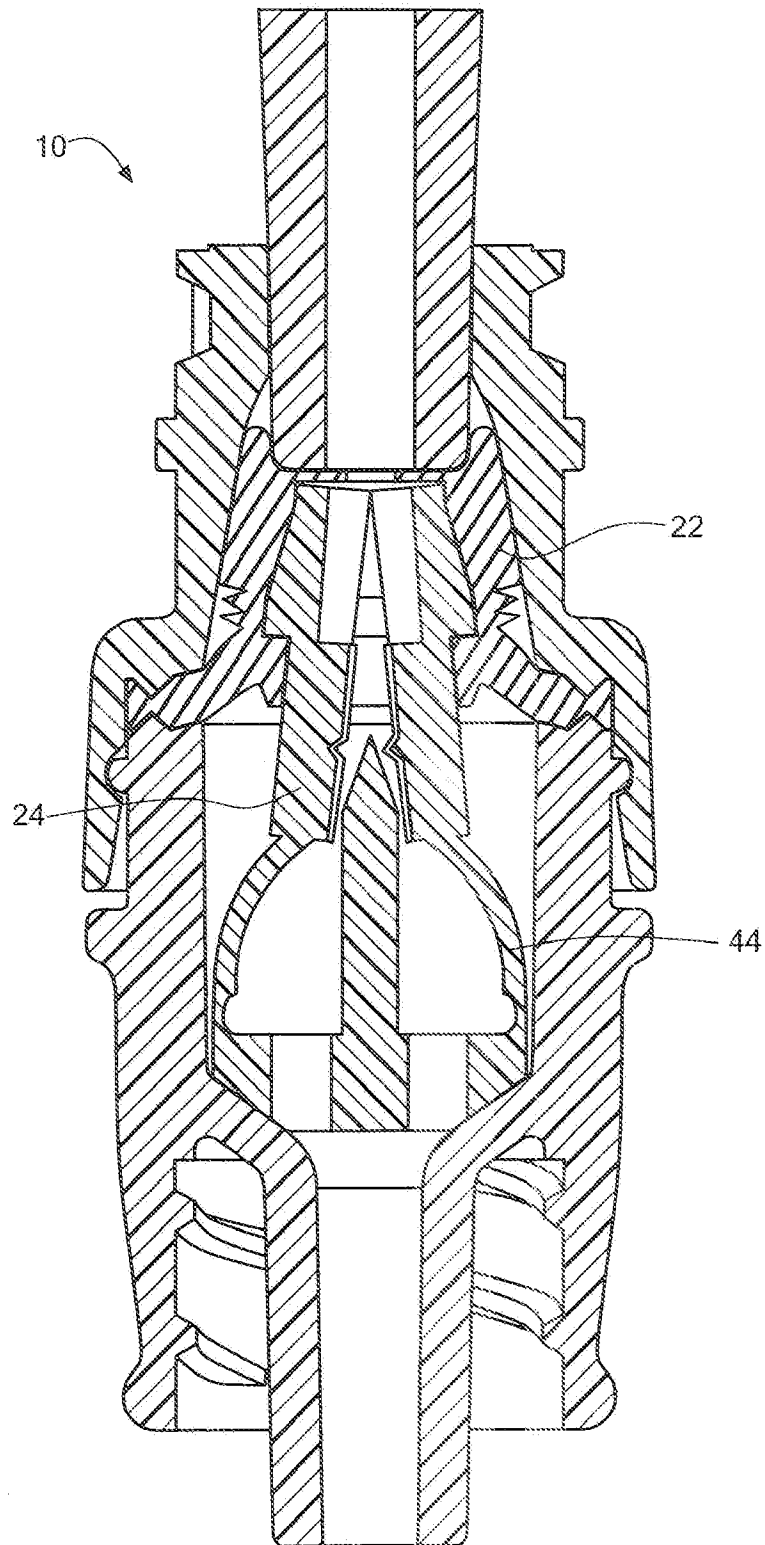


FIG. 6B

9/9

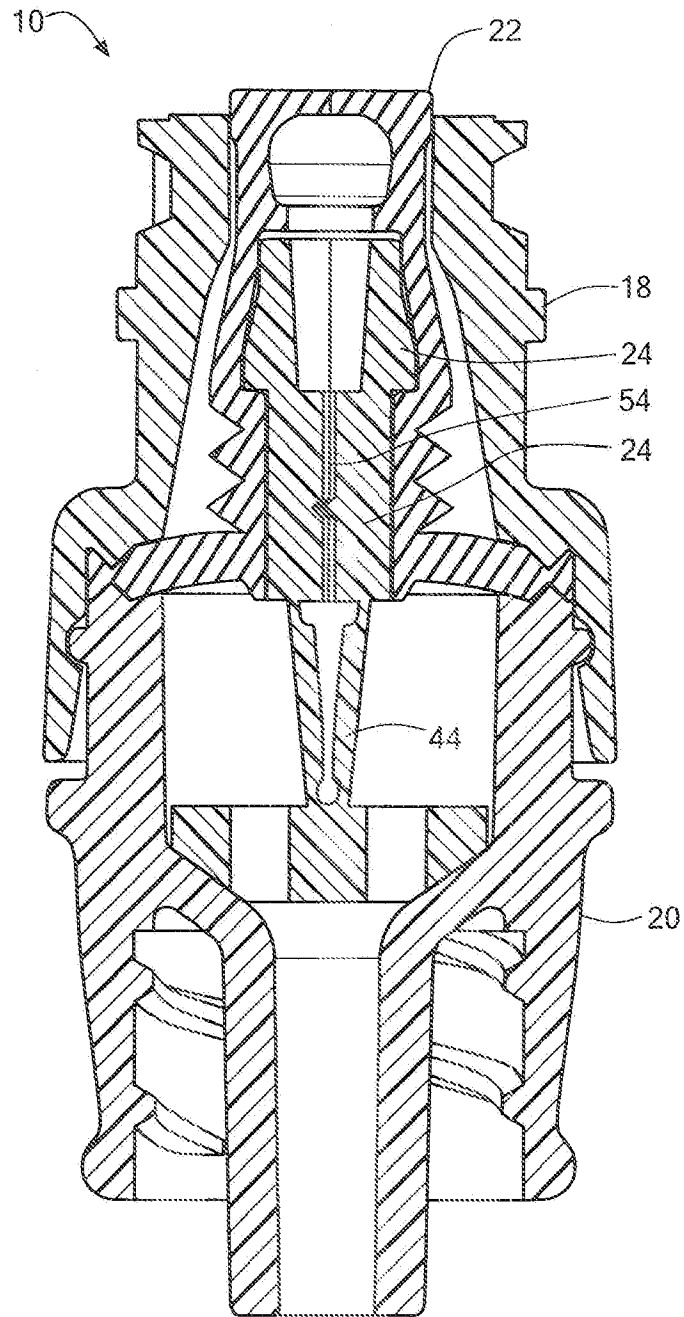


FIG. 7